

# EMC Test Report



Product : Portable Mesh Nebulizer

Model Number : Air Pro, Air Pro Plus, Air Pro 1, Air Pro 2, Air Pro 3, Air Pro 4, Air Pro 5, Air Pro 6, Air Pro 7, Air Pro 8, Air Pro 9, Air Pro 10, Air Mask 1, Air Mask 2, Air Mask 3

Prepared for : Cannapresso Health INC.  
Address : 202 North California Ave, City of Industry, CA. 91744 U.S.A.

Prepared By : Shenzhen ZCT Technology Co.,Ltd.  
Address : 3/F., Building 5, Hongsheng Industrial Zone, Bao'an Road, Xixiang Street, Bao'an District, Shenzhen, Guangdong, China.

Tel : 400-669-6965  
Fax : (86) 755-23702323

Report No. : 17ZCTE0918009ER

Date of Test : Sept.19, 2017-Sept.21, 2017

Date of Rep. : Sept.22, 2017

Prepared by(Engineer):

Reviewer(Quality Manager):

Approved & Authorized Signer(Manager):



# 1 Contents

	Page
<b>COVER PAGE</b>	
<b>1 CONTENTS</b> .....	<b>2</b>
<b>2 TEST SUMMARY</b> .....	<b>4</b>
<b>3 GENERAL INFORMATION</b> .....	<b>5</b>
3.1 GENERAL DESCRIPTION OF EUT.....	5
<b>4 EQUIPMENTS LIST FOR ALL TEST ITEMS</b> .....	<b>6</b>
<b>5 EMISSION TEST RESULTS</b> .....	<b>7</b>
5.1 MAINS TERMINALS DISTURBANCE VOLTAGE MEASUREMENT.....	7
5.1.1 E.U.T. Operation.....	7
5.1.2 Test Specification.....	7
5.1.3 Measurement Data.....	7
5.2 DISTURBANCE POWER MEASUREMENT.....	8
5.2.1 E.U.T. Operation.....	8
5.2.2 Test Specification.....	8
5.2.3 Measurement Data.....	8
5.3 RADIATED EMISSIONS MEASUREMENT.....	9
5.3.1 E.U.T. Operation.....	9
5.3.2 Test Specification.....	9
5.3.3 Measurement Data.....	9
5.4 HARMONICS.....	12
5.4.1 E.U.T. Operation.....	12
5.4.2 Test specification.....	12
5.4.3 Measurement Data.....	12
5.5 VOLTAGE CHANGES, VOLTAGE FLUCTUATIONS AND FLICKER.....	13
5.5.1 E.U.T. Operation.....	13
5.5.2 Test specification.....	13
5.5.3 Measurement Data.....	13
<b>6 IMMUNITY TEST RESULTS</b> .....	<b>14</b>
6.1 ELECTROSTATIC DISCHARGE IMMUNITY TEST.....	14
6.1.1 E.U.T. Operation.....	14
6.1.2 Test specification.....	14
6.1.3 Measurement Data.....	15
6.2 RF FIELD STRENGTH IMMUNITY TEST.....	16
6.2.1 E.U.T. Operation.....	16
6.2.2 Test specification.....	16
6.2.3 Measurement Data.....	17
6.3 ELECTRICAL FAST TRANSIENT/BURST IMMUNITY TEST.....	18
6.3.1 E.U.T. Operation.....	18
6.3.2 Test specification.....	18
6.3.3 Measurement Data.....	18
6.4 SURGE IMMUNITY TEST.....	19
6.4.1 E.U.T. Operation.....	19
6.4.2 Test specification.....	19
6.4.3 Measurement Data.....	19
6.5 CONDUCTED DISTURBANCE IMMUNITY TEST.....	20
6.5.1 E.U.T. Operation.....	20
6.5.2 Test specification.....	20
6.5.3 Measurement Data.....	20

6.6 VOLTAGE DIPS AND INTERRUPTIONS IMMUNITY TEST.....	21
6.6.1 E.U.T. Operation.....	21
6.6.2 Test specification.....	21
6.6.3 Measurement Data.....	21
<b>7 APPENDIX-PHOTOGRAPHS OF EUT CONSTRUCTIONAL DETAILS.....</b>	<b>22</b>



## 2 Test Summary

Test procedures according to the technical standards:

<u>EMC Emission</u>				
Standard	Test Item	Limit	Judgment	Remark
EN 55014-1:2017	Conducted Emission	Class B	N/A	
	Disturbance Power	-----	N/A	
	Radiated Emission	Class B	PASS	
EN 61000-3-2:2014	Harmonic Current Emission	Class A or D NOTE (2)	N/A	
EN 61000-3-3:2013	Voltage Fluctuations & Flicker	-----	N/A	
<u>EMC Immunity</u>				
Section EN55014-2:2015	Test Item	Performance Criteria	Judgment	Remark
EN 61000-4-2:2009	Electrostatic Discharge	B	PASS	
EN 61000-4-3:2006/A2:2010	RF electromagnetic field	A	PASS	
EN 61000-4-4:2012	Fast transients	B	N/A	
EN 61000-4-5:2014	Surges	B	N/A	
EN 61000-4-6:2014/AC:2015	Injected Current	A	N/A	
EN 61000-4-11: 2004	Volt. Interruptions Volt. Dips	C / C / C NOTE (3)	N/A	

**NOTE:**

(1)' N/A' denotes test is not applicable in this Test Report

(2) No limits apply for equipment with an active input power up to and including 75W.

(3)Voltage dip: 0% reduction – Performance Criteria **C**

Voltage dip: 30% reduction – Performance Criteria **C**

Voltage dip: 60% reduction – Performance Criteria **C**

For client's request and manual description, the test will not be executed.

### 3 General Information

#### 3.1 General Description Of EUT

Manufacturer:	Cannapresso Health INC.
Manufacturer Address:	202 North California Ave, City of Industry, CA. 91744 U.S.A.
EUT Name:	Portable Mesh Nebulizer
Test Model No:	Air Pro
Serial No:	Air Pro Plus, Air Pro 1, Air Pro 2, Air Pro 3, Air Pro 4, Air Pro 5, Air Pro 6, Air Pro 7, Air Pro 8, Air Pro 9, Air Pro 10, Air Mask 1, Air Mask 2, Air Mask 3
Brand Name:	
Power Supply Range:	Input: :DC 5V 1A
Test Power Supply:	Input: :DC 5V 1A

## 4 Equipments List For All Test Items

No.	Equipment	Manufacturer	Model No.	S/N	Cal date
1	EMI Test Receiver	R&S	ESCI	100612	2017-05-31
2	EMI Test Receiver	R&S	ESPI	100067	2017-05-31
3	Amplifier	HP	8447D	1937A02415	2017-05-31
4	Single Power Conductor Module	FCC	FCC-LISN-5-50-1-01-CISPR25	07118	2017-05-31
5	TRILOG Broadband Test-Antenna	SCHWARZBECK	VULB9163	9163-387	2017-05-31
6	Horn Antenna	SCHWARZBECK	BBHA9120A	B08000991-0021	2017-05-31
7	High Field Biconical Antenna	ELECTRO-METRICS	EM-6913	169	2017-05-31
8	Log Periodic Antenna	ELECTRO-METRICS	EM-6950	818	2017-05-31
9	Remote Active Vertical Antenna	ELECTRO-METRICS	EM-6892	354	2017-05-31
10	Power Clamp	SCHWARZBECK	MDS-21	3898	2017-05-31
11	Single Power Conductor Module	FCC	FCC-LISN-5-50-1-01-CISPR25	07254	2017-05-31
12	Teo Line Single Phase Module	SCHWARZBECK	NSLK8128	D-69124	2017-05-31
13	Positioning Controller	C&C	CC-C-1F	MF7802155	2017-05-31
14	Electrostatic Discharge Simulator	TESEQ	NSG437	128	2017-05-31
15	Fast Transient Burst Generator	SCHAFFNER	MODULA6150	34587	2017-05-31
16	Fast Transient Noise Simulator	Noiseken	FNS-105AX	31438	2017-05-31
17	Capacitive Coupling Clamp	TESEQ	CDN8014	25115	2017-05-31
18	Color TV Pattern Generator	PHILIPS	PM5418	TM209966	N/A
19	Power Frequency Magnetic Field Gene	EVERFINE	EMS61000-8K	608085	2017-05-31
20	Triple-Loop Antenna	EVERFINE	LLA-2	607035	2017-05-31
21	10dB attenuator	SCHWARZBECK	MTAIMP-136	R65.90.0009	2017-05-31
22	AC Power Source	California Instrumnets	5001ix-400-N0	HK53570	2017-05-31
23	Power Analyzer	California Instrumnets	PACS-1	X71719	2017-05-31



<b>5 Emission Test Results</b>						
<b>5.1 Mains Terminals Disturbance Voltage Measurement</b>						
Frequency Range:	150kHz to 30MHz					
Limits:	Table 1 of EN 55014-1					
Detector:	Peak for pre-scan (9kHz Resolution Bandwidth) Quasi-Peak & Average if maximized peak within 6dB of Average Limit					
<b>5.1.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>5.1.2 Test Specification</b>						
<p>EUT was placed upon a wooden test table 0.8m above the horizontal metal plane and 0.4m from the vertical metal reference plane, and it was connected to an AMN. The closest distance between the boundary of the EUT and the surface of the AMN is 0.8m, All peripherals were connected to another AMN, and placed at a distance of 10 cm from each other. A spectrum and receiver was connected to the RF output port of the AMN. Both average and quasi-peak value were detected.</p>						

Associated with the conducted emission test data in this report is a  $\pm 1.54$ dB measurement uncertainty.

<b>5.1.3 Measurement Data</b>
<p>An initial pre-scan was performed on the live and neutral lines.</p> <p>Quasi-peak or average measurements were performed at the frequency which maximum peak emissions were detected.</p> <p>Please refer to the attached quasi-peak &amp; average measurement data for reference.</p>
N/A

<b>5.2 Disturbance Power Measurement</b>						
Frequency Range:		30MHz to 300MHz				
Limits:		Table 2 of EN55014-1				
Detector:		Peak for pre-scan (120kHz resolution bandwidth)				
		Quasi-Peak and Average if maximum peak within 6dB of limit				
<b>5.2.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.2 °C	Humidity:	55% RH	Atmospheric Pressure:	102	Kpa
EUT Operation:	Normal Operation					
<b>5.2.2 Test Specification</b>						
The EUT was placed on a wooden table which is 0.8m in height. A non-metallic slide groove 6m long was placed at the same height for movement of the absorbing clamp. Absorbing clamp moved along the slide groove during testing to find the maximum disturbance reading. All reflecting or absorbing objects are not closer than 0.8m to the measuring set-up.						
Associated with the radiated emission test data in this report is a $\pm 3.44$ dB measurement uncertainty.						
<b>5.2.3 Measurement Data</b>						
An initial pre-scan was performed on the live and neutral lines. Quasi-peak or average measurements were performed at the frequency which maximum peak emissions were detected. Please refer to the attached quasi-peak & average measurement data.						
N/A						



### 5.3 Radiated Emissions Measurement

Frequency Range:	30MHz to 1000MHz
Limits:	Table 2 of EN55014-1
Detector:	Peak for pre-scan (120kHz resolution bandwidth)
	Quasi-Peak and Average if maximum peak within 6dB of limit

#### 5.3.1 E.U.T. Operation

Operating Environment:

Temperature:	24.1 °C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					

#### 5.3.2 Test Specification

EUT was placed upon a wooden test table which was placed on the turn table 0.8m above the horizontal metal ground plane, and operating in the mode as mentioned above. A receiving antenna was placed 3m away from the EUT. During testing, turn around the turn table and move the antenna from 1m to 4m to find the maximum field-strength reading. All peripherals were placed at a distance of 10cm between each other. Both horizontal and vertical antenna polarities were tested.


Associated with the radiated emission test data in this report is a  $\pm 3.08$ dB measurement uncertainty.

#### 5.3.3 Measurement Data

An initial pre-scan was performed in the 3m chamber using the spectrum analyzers in peak detection mode. The EUT was measured by Biology antenna with 2 orthogonal polarities and peak emissions from the EUT were detected within 6dB of the class B limit line.


The following quasi-peak measurements were performed on the EUT.

<b>EUT:</b>	Portable Mesh Nebulizer	<b>Model No.:</b>	Air Pro
<b>Temperature:</b>	24.1 °C	<b>Relative Humidity:</b>	55%
<b>Distance:</b>	3m	<b>Test Power:</b>	DC 5V
<b>Polarization:</b>	Horizontal	<b>Test Result:</b>	Pass
<b>Standard:</b>	EN 55014 3M Radiaton	<b>Test By:</b>	King
<b>Note:</b>	Normal Operation		

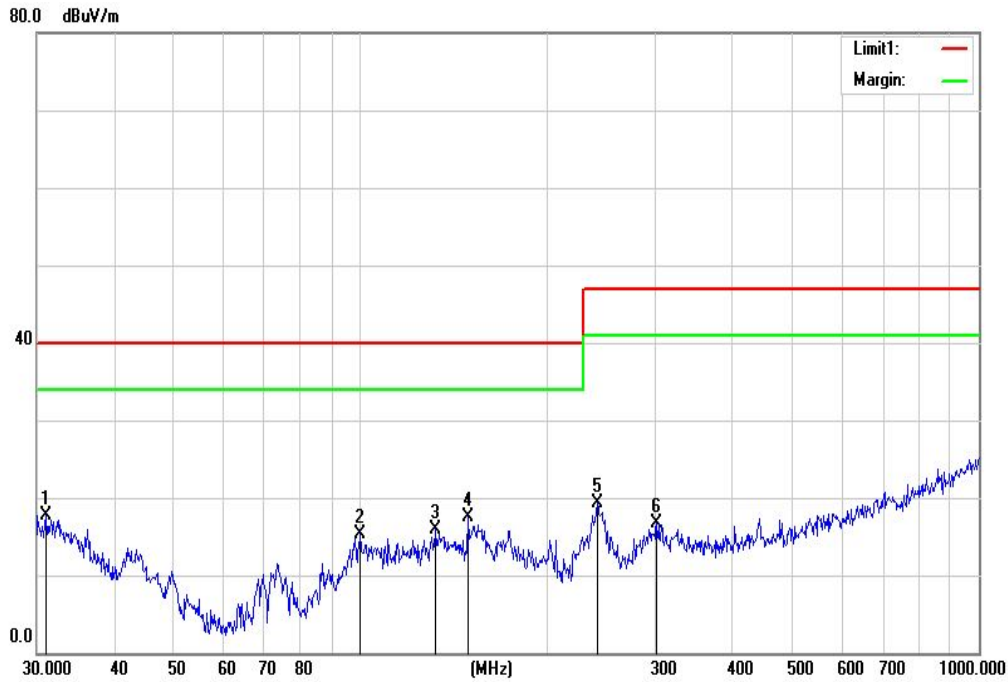

No.	Frequency (MHz)	Reading (dBuV)	Correct Factor(dB/m)	Result (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Remark
1*	31.0706	27.57	-9.83	17.74	40.00	-22.26	QP
2	99.8777	33.39	-18.12	15.27	40.00	-24.73	QP
3	132.2206	30.47	-14.56	15.91	40.00	-24.09	QP
4	149.4857	33.02	-15.52	17.50	40.00	-22.50	QP
5	241.6763	35.68	-16.40	19.28	47.00	-27.72	QP
6	301.4224	30.05	-13.35	16.70	47.00	-30.30	QP

<b>EUT:</b>	Portable Mesh Nebulizer	<b>Model No.:</b>	Air Pro
<b>Temperature:</b>	24.1°C	<b>Relative Humidity:</b>	55%
<b>Distance:</b>	3m	<b>Test Power:</b>	DC 5V
<b>Polarization:</b>	Vertical	<b>Test Result:</b>	Pass
<b>Standard:</b>	EN 55014 3M Radiaton	<b>Test By:</b>	King
<b>Note:</b>	Normal Operation		

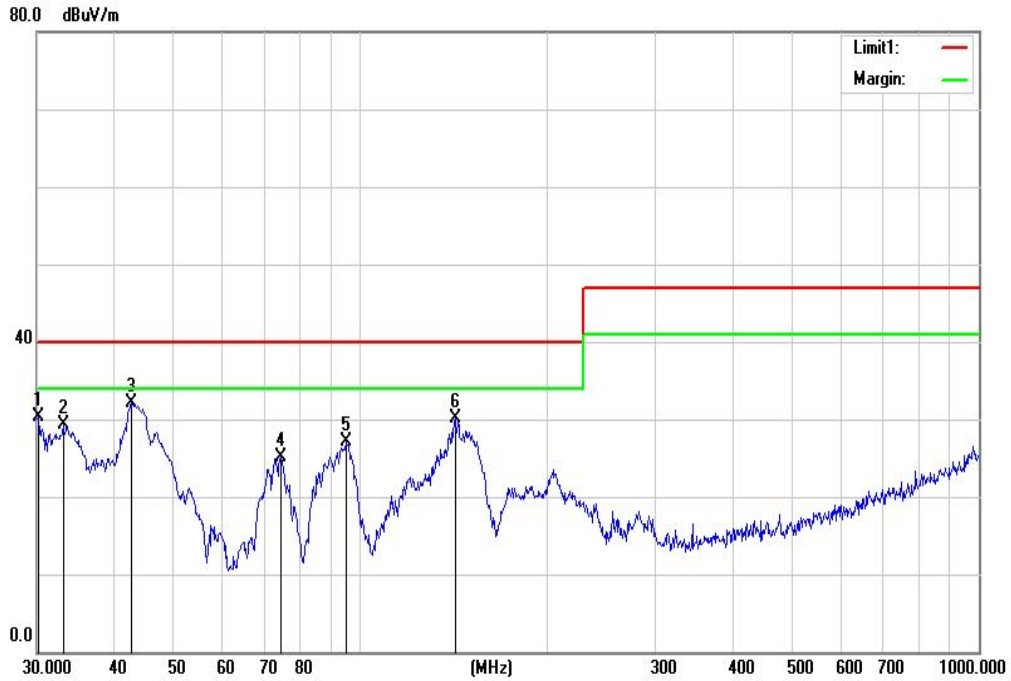

No.	Frequency (MHz)	Reading (dBuV)	Correct Factor(dB/m)	Result (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Remark
1	30.2111	39.53	-9.29	30.24	40.00	-9.76	QP
2	33.0950	40.44	-11.10	29.34	40.00	-10.66	QP
3*	42.6000	49.63	-17.51	32.12	40.00	-7.88	QP
4	74.3955	47.66	-22.59	25.07	40.00	-14.93	QP
5	94.7601	46.60	-19.40	27.20	40.00	-12.80	QP
6	142.3244	45.16	-15.13	30.03	40.00	-9.97	QP

<b>5.4 Harmonics</b>						
Frequency Range:		100Hz to 2kHz				
Test Requirement:		EN 61000-3-2				
<b>5.4.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.2°C	Humidity:	56% RH	Atmospheric Pressure:	102.0	Kpa
EUT Operation:	Normal Operation					
<b>5.4.2 Test specification</b>						
EUT operated in the mode as mentioned above, and connected to Harmonic/Flicker measuring equipment which was connected to an AC power source. Measurement was performed after EUT operating in static state for 10 seconds. Each order harmonics found to meet the relevant limits.						
<b>5.4.3 Measurement Data</b>						
N/A						

<b>5.5 Voltage changes, voltage fluctuations and flicker</b>						
Test Requirement:		EN 61000-3-3				
<b>5.5.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.2°C	Humidity:	56% RH	Atmospheric Pressure:	102.0	Kpa
EUT Operation:	Normal Operation					
<b>5.5.2 Test specification</b>						
EUT was operated in the mode as mentioned above, and connected to Harmonic/Flicker measuring equipment which was connected to an AC power source.						
<b>5.5.3 Measurement Data</b>						
N/A						

<b>6 Immunity Test Results</b>						
<b>6.1 Electrostatic discharge immunity test</b>						
Acceptable Performance Criterion:	B					
Discharge Impedance:	330 Ω / 150 pF					
Discharge Voltage:	Air Discharge:		±8 kV			
	Contact Discharge:		±4 kV			
	VCP, HCP:		±4 kV			
Polarity:	Positive & Negative					
Minimum discharge Interval:	1 second					
<b>6.1.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.2°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>6.1.2 Test specification</b>						
<p>EUT was operated in the mode as mentioned above,. Both contact and air discharge was executed. contact discharge to the conductive surfaces and to coupling planes; air discharge at insulating surfaces. Each test point shall be subjected to 10 discharges at least (For each Level and polarity).</p>						



### 6.1.3 Measurement Data

#### Test Record

Electrostatic Discharge Immunity Test Results				
Applicant: <u>Cannapresso Health INC.</u>			Test Date: <u>Sept.20, 2017</u>	
EUT: <u>Portable Mesh Nebulizer</u>			Test Result: <input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail	
M/N: <u>Air Pro</u>			Temp: <u>24.2</u> °C , Humi: <u>54</u> %	
Power Supply: <u>Input: DC 5V</u>			Atmospheric Pressure: <u>101.0</u> Kpa	
Operating Mode	Normal Operation			Criterion
Test Level	Air Discharge(A) <u>± 8</u> KV , Contact Discharge (C) <u>± 4;</u> KV			
Test Position	Discharge Mode	Points	Discharge times for each Point (for each Level And polarity)	Result
Shell	A	4	10	Pass
HCP	C	4	10	Pass
VCP	C	4	10	Pass
Button	A	4	10	Pass
Screw	C	4	10	Pass
Note: "A" means Air Discharge, "C" means Contact Discharge, Horizontal Coupling Plane(HCP) and Vertical Coupling plane(VCP).				

<b>6.2 RF field strength immunity test</b>						
Acceptable Performance Criterion:	A					
Test Level	3 V/m					
Test Distance	3 m					
Frequency Range	80MHz~1000MHz					
Polarity:	Horizontal & Vertical					
<b>6.2.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.1°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>6.2.2 Test specification</b>						
<p>Test was executed in a fully Anechoic chamber. An antenna was used to transmit interference signal. EUT was placed upon a wooden table above the reference ground 0.8m, and was positioned so that the four sides of the EUT shall be exposed to the electromagnetic field in a sequence, In each position the performance of the EUT was investigated. A camera was used to monitor the loss of function or degradation of performance of the EUT.</p>						

This test item was transferred to Shenzhen Academy of Metrology and Quality Inspection (SMQ) which was confirmed to have enough capacity to perform this subcontract work.

### 6.2.3 Measurement Data

### Test Record

Radiated Frequency Field Strength Immunity Test Results					
Applicant: <u>Cannapresso Health INC.</u>			Test Date: <u>Sept.21, 2017</u>		
EUT: <u>Portable Mesh Nebulizer</u>			Test Result: <input checked="" type="checkbox"/> Pass <input type="checkbox"/> Fail		
M/N: <u>Air Pro</u>			Temp: <u>24.1</u> °C , Humi: <u>55</u> %		
Power Supply: <u>Input: DC 5V</u>			Atmospheric Pressure: <u>101.0</u> Kpa		
Test Port	Input Port				
Operating Mode	Normal Operation				
Test Level	<u>3</u> V/m (r.m.s) ( unmodulated )			Criterion	A
Frequency Range(MHz)	Antenna polarity	Modulation	EUT position	Result	
80~1000	Horizontal	1kHz, 80%, AM	Front	Pass	
			Rear	Pass	
			Left	Pass	
			Right	Pass	
80~1000	Vertical	1kHz, 80%, AM	Front	Pass	
			Rear	Pass	
			Left	Pass	
			Right	Pass	
Note : None					

<b>6.3 Electrical fast transient/burst immunity test</b>						
Acceptable Performance Criterion:	B					
Test Level:	0.5, 1.0, kV on AC Line; 0.5 kV on Signal Line					
Repetition Frequency:	5 kHz					
Burst Duration:	300 ms					
Test Duration:	2 minute for each level & polarity					
<b>6.3.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.1°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>6.3.2 Test specification</b>						
EUT was placed on a metal ground reference plane and was insulated from it by a wooden support which is 0.1m thick. The ground reference plane is connected to the protective earth. The test generator and the coupling/decoupling network were placed directly on, and bonded to the ground reference plane.						
<b>6.3.3 Measurement Data</b>						
N/A						

<b>6.4 Surge immunity test</b>						
Acceptable Performance Criterion:	B					
Test Level:	0.5, 1kV Live to Neutral					
	0.5, 1, 2kV Live, Neutral to Earth					
Polarity:	Positive & Negative					
Generator source impedance:	2 $\Omega$ & 12 $\Omega$					
Trigger Mode:	Internal					
No. of surges:	5 positive, 5 negative at 0°, 90°, 180°, 270°.					
<b>6.4.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24.2°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>6.4.2 Test specification</b>						
EUT was placed on a wooden table which is 0.8m above the ground and operated in the mode as mentioned above,. The power cord between the EUT and the coupling/decoupling network was bundled so as to make it less than 2 m in length.						
<b>6.4.3 Measurement Data</b>						
N/A						

<b>6.5 Conducted disturbance immunity Test</b>						
Acceptable Performance Criterion:	A					
Test Level	3 V					
Frequency Range	0.150MHz~80MHz					
<b>6.5.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>6.5.2 Test specification</b>						
<p>The equipment to be tested was placed on an insulating support of 0,1 m height above a ground reference plane. The minimum distance between the EUT and all other conductive structures, except the ground reference plane is more than 0,5 m. All relevant cables were provided with the appropriate coupling and decoupling devices at a distance between 0,1 m and 0,3 m from the projected geometry of the EUT .</p>						
<b>6.5.3 Measurement Data</b>						
N/A						



<b>6.6 Voltage dips and interruptions immunity test</b>						
Acceptable Performance Criterion:		B & C				
Test Level:		< 5% of $U_T$ (Supply Voltage) for 0.5 and 250 Periods				
		70 % of $U_T$ (Supply Voltage) for 25 Periods				
No. of Dips / Interruptions:		3 per Level				
<b>6.6.1 E.U.T. Operation</b>						
Operating Environment:						
Temperature:	24°C	Humidity:	55% RH	Atmospheric Pressure:	101.0	Kpa
EUT Operation:	Normal Operation					
<b>6.6.2 Test specification</b>						
<p>EUT connected to the test generator with the shortest power supply cable as specified by the EUT manufacturer. The rated voltage of the EUT was used as the basis for voltage test level specification. After each group of tests, a full functional check was performed.</p>						
<b>6.6.3 Measurement Data</b>						
N/A						

## 7 APPENDIX-Photographs Of EUT Constructional Details



Photo 1



Photo 2

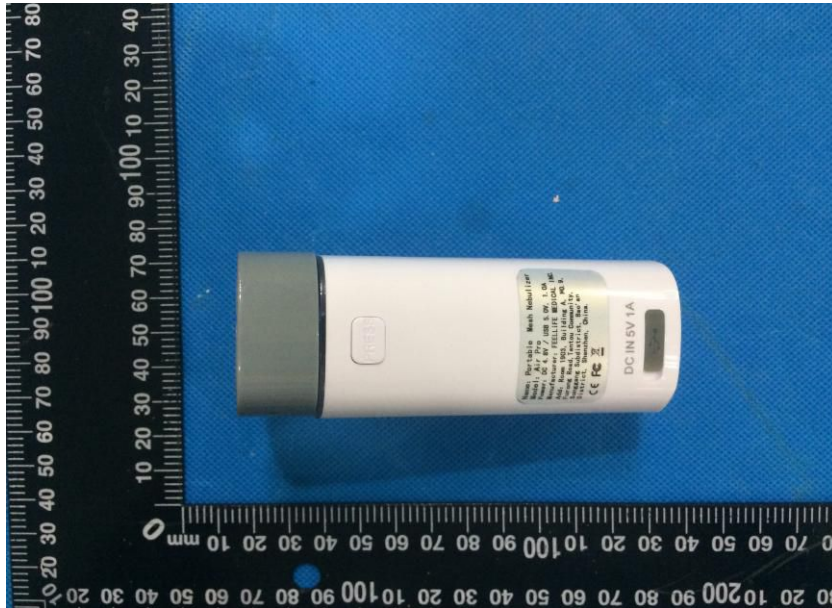


Photo 3



Photo 4





Photo 5

--End of report--

