



Customer: Cannapresso Health Inc.
 Customer Sample ID: Cannapresso iPrefer Disposable Devise 50mg/mL series
 Laboratory Number: 20C0084-01

Density: 1.045




Cannabinoid Profile

Extraction Technician: RH
 Analytical Chemist: MF

Extraction Date(s)	Analysis Date(s)
3/9/2020	3/9/2020

Cannabinoids (HPLC)		Results	
	LOD (mg/mL)	%	mg/mL
Cannabidivarin (CBDV)	<0.20		
Cannabidiolic Acid (CBD-A)	<0.20		
Cannabigerolic Acid (CBG-A)	<0.20		
Cannabigerol (CBG)	<0.20		
Cannabidiol (CBD)		5.26	52.6
Tetrahydrocannabivarin (THCV)	<0.20		
Cannabinol (CBN)	<0.20		
delta 9-Tetrahydrocannabinol (THC)	<0.20		
delta 8-Tetrahydrocannabidol	<0.20		
Cannabichromene (CBC)	<0.20		
delta-9-Tetrahydrocannabinolic Acid (THC-A)	<0.20		
Cannabinoids Total		%	mg/mL
Max Active THC		0.00	0.00
Max Active CBD		5.26	52.60
T.Active Cannabinoids		5.26	52.60
Total Cannabinoids		5.26	52.60
Ratios			
NA:1 CBD to THC		0.00:1 THC to CBD	

Cannabinoid (mg/mL)

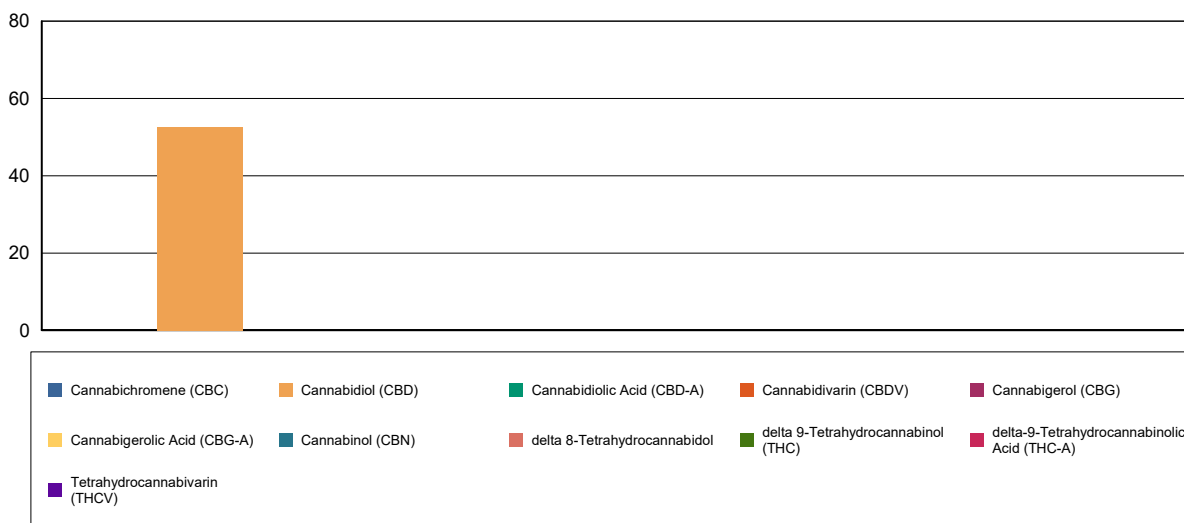

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods . The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



Customer: Cannapresso Health Inc.
Customer Sample ID: Cannapresso iPrefer Disposable Devise 50mg/mL series
Laboratory Number: 20C0084-01

Density: 1.045



Residual Solvents Profile

Extraction Technician: RH
 Analytical Chemist: CB

Extraction Date(s)	Analysis Date(s)
3/9/2020	3/9/2020

Residual Solvents	Results	Calibration Range
	ug/mL	
Propane	<98.0	100 - 2000
Isobutane	<98.0	100 - 2000
Methanol	<98.0	100 - 2000
Butane	<98.0	100 - 2000
Isopropanol	<98.0	100 - 2000
Ethanol	<98.0	100 - 2000
2-Methyl Butane	<98.0	100 - 2000
Acetonitrile	<98.0	100 - 2000
Acetone	<98.0	100 - 2000
n-Pentane	<98.0	100 - 2000
n-Hexane	<49.0	50 - 2000
Tetrahydrofuran	<98.0	100 - 2000
Benzene	<0.980	1.0 - 50
n-Heptane	<98.0	100 - 2000
Toluene	<98.0	100 - 2000
Ethylbenzene	<98.0	100 - 2000
m+p Xylene	<98.0	100 - 2000
o-Xylene	<98.0	100 - 2000
Total Xylenes	<98.0	100 - 2000
1,2,3-Trimethylbenzene	<98.0	100 - 2000

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods . The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



Customer: Cannapresso Health Inc.
Customer Sample ID: Cannapresso iPrefer Disposable Devise 150mg/mL series
Laboratory Number: 20C0084-02

Density: 1.045




Cannabinoid Profile

Extraction Technician: RH
Analytical Chemist: MF

Extraction Date(s)	Analysis Date(s)
3/9/2020	3/9/2020

Cannabinoids (HPLC)		Results	
	LOD (mg/mL)	%	mg/mL
Cannabidivarin (CBDV)	<0.20		
Cannabidiolic Acid (CBD-A)	<0.20		
Cannabigerolic Acid (CBG-A)	<0.20		
Cannabigerol (CBG)	<0.20		
Cannabidiol (CBD)		14.34	143
Tetrahydrocannabivarin (THCV)	<0.20		
Cannabinol (CBN)	<0.20		
delta 9-Tetrahydrocannabinol (THC)	<0.20		
delta 8-Tetrahydrocannabidol	<0.20		
Cannabichromene (CBC)	<0.20		
delta-9-Tetrahydrocannabinolic Acid (THC-A)	<0.20		
Cannabinoids Total		%	mg/mL
Max Active THC		0.00	0.00
Max Active CBD		14.30	143.00
T.Active Cannabinoids		14.30	143.00
Total Cannabinoids		14.30	143.00
Ratios			
NA:1 CBD to THC		0.00:1 THC to CBD	

Cannabinoid (mg/mL)

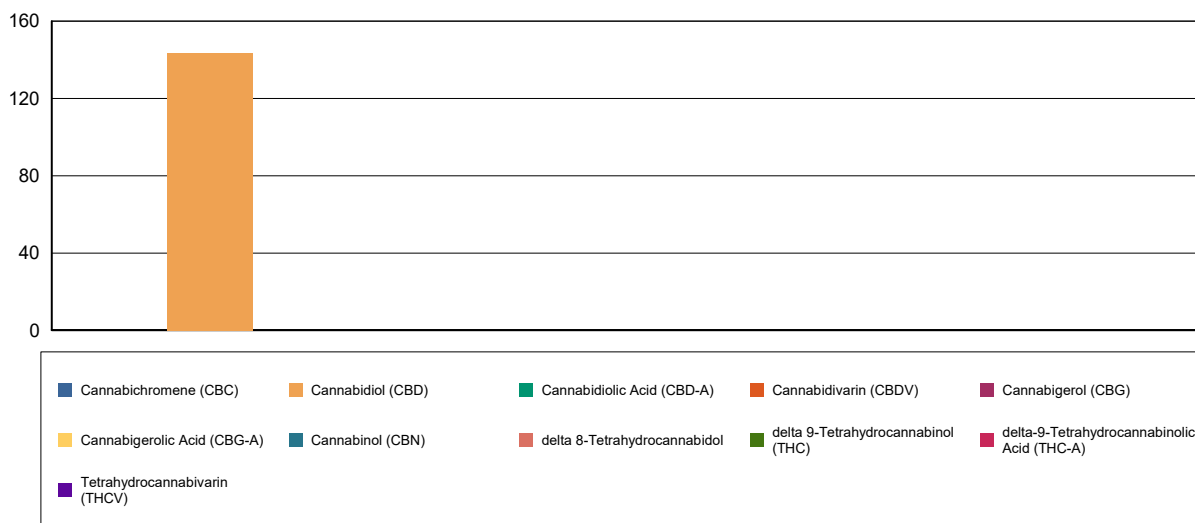

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



Customer: Cannapresso Health Inc.
Customer Sample ID: Cannapresso iPrefer Disposable Devise 150mg/mL series
Laboratory Number: 20C0084-02

Density: 1.045



Residual Solvents Profile

Extraction Technician: RH
 Analytical Chemist: CB

Extraction Date(s)	Analysis Date(s)
3/9/2020	3/9/2020

Residual Solvents	Results	Calibration Range
	ug/mL	
Propane	<102	100 - 2000
Isobutane	<102	100 - 2000
Methanol	<102	100 - 2000
Butane	<102	100 - 2000
Isopropanol	<102	100 - 2000
Ethanol	<102	100 - 2000
2-Methyl Butane	<102	100 - 2000
Acetonitrile	<102	100 - 2000
Acetone	<102	100 - 2000
n-Pentane	<102	100 - 2000
n-Hexane	<50.8	50 - 2000
Tetrahydrofuran	<102	100 - 2000
Benzene	<1.02	1.0 - 50
n-Heptane	<102	100 - 2000
Toluene	<102	100 - 2000
Ethylbenzene	<102	100 - 2000
m+p Xylene	<102	100 - 2000
o-Xylene	<102	100 - 2000
Total Xylenes	<102	100 - 2000
1,2,3-Trimethylbenzene	<102	100 - 2000

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods . The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.